

KRIBIOLISA™ E.coli HCP (Wide Coverage) ELISA

REF : KBBP13200

Ver 1.0

RUO

Enzyme Immunoassay for the Quantitative Determination of E.coli HCP (Wide Coverage) originated from BL21.

RUO	For Research Use Only	REF	Catalog Number
	Store At	LOT	Batch Code
	Manufactured By		Biological Risk
	Expiry Date		Consult Operating Instructions

For Research Use Only. Purchase does not include or carry the right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of KRISHGEN BioSystems is strictly prohibited.

REF KBBP13200  96 tests

KRISHGEN BioSystems

For US/Europe Customers: toll free +1(888)-970-0827 | tel +1(562)-568-5005

For Asia/India Customers: +91(22)-49198700

Email: sales1@krishgen.com | <http://www.krishgen.biz> / www.krishgenbio.com

Introduction:

The KRIBIOLISA™ ELISA kits are used for assessing the specific biomarker in samples analytes which may be serum, plasma and cell culture supernatant as validated with the kit. The kit employs a sandwich ELISA technique which leads to a higher specificity and increased sensitivity compared to conventional competitive ELISA kits which employ only one antibody. Double antibodies are used in this kit.

Intended Use:

The KRIBIOLISA™ E.coli HCP (Wide Coverage) ELISA kit is intended for use in determining the presence of host cell proteins (HCPs) in products manufactured by expression in E.coli HCP (Wide Coverage) originated from BL21, such as interleukin (IL), recombinant human interferon (rhIFN), recombinant human granulocyte-macrophage colony-stimulating factor (rhGM-CSF), recombinant human tumor necrosis factor (rhTNF), growth-promoting factor (EGF/FGF/PDGF), et.al.

Principle:

The method employs sandwich ELISA technique. Polyclonal antibodies are pre-coated onto microwells. Samples, standards, Anti-E.coli HCP (Wide Coverage) HRP conjugate are pipetted into microwells and incubated to form a immune complex. After washing microwells in order to remove any non-specific binding, the substrate solution (TMB) is added to microwells and color develops proportionally to the amount of E.coli HCP (Wide Coverage) in the sample. Color development is then stopped by addition of stop solution. Absorbance is measured at 450 nm.

Materials Provided:

1. E.coli HCP Antibody Coated Microtiter Plate (12 x 8 wells) - 1 no
2. E.coli HCP Standard (lyophilized, concentration indicated on the vial) - 2 vials
3. Anti-E.coli HCP:HRP Conjugate (concentrated) - 120 ul
4. Standard Diluent – 1.5 ml
5. Assay Diluent - 2 x 25 ml
6. (10X) Wash Buffer – 2 x 25 ml
7. TMB Substrate - 12 ml
8. Stop Solution - 12 ml
9. Instruction Manual

Materials to be provided by the End-User:

1. Microtiter Plate Reader able to measure absorbance at 450 nm.
2. Adjustable pipettes and multichannel pipettor to measure volumes ranging from 25 ul to 1000 ul
3. Deionized (DI) water
4. Wash bottle or automated microplate washer
5. Clean tubes and Eppendorf tubes
6. Precision single and multi-channel pipette and disposable tips.
7. 37°C incubator
8. Timer.

Handling/Storage:

1. All reagents should be stored as indicated on the component label.
2. All the reagents and wash solutions should be used within 12 months from manufacturing date.
3. Before using, bring all components to room temperature (18-25°C). Upon assay completion ensure all components of the kit are returned to appropriate storage conditions.
4. The Substrate is light-sensitive and should be protected from direct sunlight or UV sources.



Health Hazard Warnings:

1. Reagents that contain preservatives may be harmful if ingested, inhaled or absorbed through the skin.
2. For Research Use Only.

Sample Preparation and Storage:

Test Samples: In-process, harvested bulk, drug substance and Drug Product Make sure that the samples are clear and transparent, and insoluble substances need to be removed by centrifugation or filtration.

Test Sample Preparation: The user should estimate the concentration of target protein in the test sample, and select a proper dilution factor to make the diluted target protein concentration fall in the optimal detection range of the kit. Dilute the sample with the provided assay diluent, and several trials may be necessary. The test sample must be well mixed with the assay diluent.

Reagent Preparation (all reagents should be diluted immediately prior to use):

1. Label any aliquots made with the kit Lot No and Expiration date and store it at appropriate conditions mentioned.
2. Bring all reagents to Room temperature before use.
3. To make **Wash Buffer (1X)**; dilute **25 ml of (10X) Wash Buffer in 225 ml of DI water**.
4. **Anti-E.coli HCP:HRP Conjugate Working Solution:** Dilute the Anti-E.coli HCP:HRP Conjugate with Assay Diluent at 1:100 and mix them thoroughly (i.e. Add 1 ul of Anti-E.coli HCP:HRP Conjugate into 99 ul of Assay Diluent).
6. **Standards Preparation:** Reconstitute original *E.coli* HCP Standard with 0.5 ml of Standard Diluent to get a concentration per ml as indicated on the vial label*. Keep the standard for 15 mins with gentle agitation before making further dilutions. Prepare the additional Standards by serially diluting the standard stock solution as per the below table.

*Concentration on reconstitution is indicated on the vial label. Upon reconstitution, dilute with the assay diluent to the highest concentration 243 ng/ml and then subsequently follow the dilution table below for preparation of the other standards.

Standard Concentration	Standard Vial	Dilution Particulars
0.5ml*	Lyophilized Standard	Reconstitute with 0.5 ml Assay Diluent
Dilute appropriately using the Assay Diluent to make the first concentration of 243 ng/ml.		
243 ng/ml	Standard No.7	Reconstituted Standard + Assay Diluent
81 ng/ml	Standard No.6	300 ul Standard No.7 + 600 ul Assay Diluent
27 ng/ml	Standard No.5	300 ul Standard No.6 + 600 ul Assay Diluent
9 ng/ml	Standard No.4	300 ul Standard No.5 + 600 ul Assay Diluent
3 ng/ml	Standard No.3	300 ul Standard No.4 + 600 ul Assay Diluent
1.5 ng/ml	Standard No.2	300 ul Standard No.3 + 600 ul Assay Diluent
0 ng/ml	Standard No.1	Only Assay Diluent

Procedural Notes:

1. In order to achieve good assay reproducibility and sensitivity, proper washing of the plates to remove excess un-reacted reagents is essential.
2. High Dose Hook Effect may be observed in samples with very high concentrations of E.coli HCP (Wide Coverage). High Dose Hook Effect is due to excess of antibody for very high concentrations of E.coli HCP (Wide Coverage) present in the sample.
3. E.coli HCP (Wide Coverage) concentration of the undiluted sample is less than the diluted sample, this may be indicative of the Hook Effect.
4. Avoid assay of Samples containing sodium azide (NaN_3), as it could destroy the HRP activity resulting in under-estimation of the amount of E.coli HCP (Wide Coverage).
5. It is recommended that all Standards and Samples be assayed in duplicates or triplicates.
6. Maintain a repetitive timing sequence from well to well for all the steps to ensure that the incubation timings are same for each well.

7. If the Substrate has a distinct blue color prior to use it may have been contaminated and use of such substrate can lead to compromisation of the sensitivity of the assay.
8. The plates should be read within 30 minutes after adding the Stop Solution.
9. Make a work list in order to identify the location of Standards and Samples.

Assay Procedure:

1. It is strongly recommended that all Standards and Samples be run in duplicates or triplicates. A standard curve is required for each assay.
2. Add **100 ul prepared Standards and Samples** to respective wells.
3. Add **100 ul Anti-E.coli HCP:HRP Conjugate Working Solution** to all wells. Mix well.
4. Cover the plate with a sealer and incubate for 180 minutes at room temperature on a shaker at 600rpm.
5. Aspirate and wash plate 4 times with diluted Wash Buffer (1X) and blot residual buffer by firmly tapping plate upside down on absorbent paper. Wipe of any liquid from the bottom outside of the microtiter wells as any residue can interfere in the reading step.
6. Pipette **100 ul TMB Substrate** in all the wells.
7. Incubate the plate at **room temperature** for **30 minutes**. DO NOT SHAKE or else it may result in higher backgrounds and worse precision. Positive wells should turn bluish in color.
8. Pipette **100 ul of Stop Solution** to all wells. The wells should turn from blue to yellow in color.
9. Read the absorbance at 450 nm with a microplate within 10-15 minutes after addition of Stop solution.

Calculation of Results:

Determine the Mean Absorbance for each set of duplicate or triplicate Standards and Samples. Using Graph Paper, plot the average value (absorbance 450nm) of each standard on the Y-axis versus the corresponding concentration of the standards on the X-axis. Draw the best fit curve through the standard points. To determine the unknown E.coli HCP (Wide Coverage) concentrations, find the unknown's Mean Absorbance value on the Y-axis and draw a horizontal line to the standard curve. At the point of intersection, draw a vertical line to the X-axis and read the E.coli HCP (Wide Coverage) concentration.

If samples were diluted, multiply by the appropriate dilution factor. Software which is able to generate a cubic spline curve-fit or 4-PL is best recommended for automated results.

Note:


It is recommended to repeat the assay at a different dilution factor in the following cases:

- If the sample absorbance value is below the first standard.

Typical Data

Concentration ng/ml	Abs 1	Abs 2	Abs 3	Mean Abs	Interpolated Concentration ng/ml	% Recovery
0	0.0785	0.0838	0.0824	0.0816	-	-
1.5	0.1211	0.1197	0.1189	0.1199	1.67	111.58
3	0.1433	0.1487	0.1486	0.1469	2.94	98.12
9	0.2666	0.2767	0.3059	0.2831	9.37	104.08
27	0.5843	0.6005	0.6172	0.6007	26.51	98.19
81	1.2211	1.2672	1.2158	1.2347	81.49	100.61
243	1.8935	1.8819	1.9061	1.8938	242.52	99.80

Typical Graph

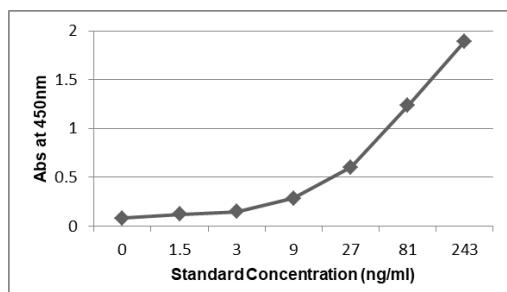

Abs = absorbance at 450nm

Quality Control:

It is recommended that for each laboratory assay appropriate quality control samples in each run to be used to ensure that all reagents and procedures are correct.

Performance Characteristics of the Kit:

This kit has been validated. Please view the details herein below.

Standard Calibration Range:

1.5 ng/ml – 243 ng/ml

Sensitivity:

Limit of Quantification: It is defined as the lowest detectable concentration that can be determined with an acceptable repeatability and the LOQ was found to be 0.95 ng/ml.

Specificity:

This assay has high sensitivity and excellent specificity for detection of E.coli HCP (Wide Coverage). No significant cross-reactivity or interference with CHO, Vero, HEK293T, Hansenula Polymorpha HCP's.

Precision

Precision is defined as the percent coefficient of variation (%CV) i.e. standard deviation divided by the mean and multiplied by 100. Assay precision was determined by both intra (n=5 assays) and inter assay (n=5 assays) reproducibility on two pools with low (3 ng/ml) and high (81 ng/ml) concentrations. While actual precision may vary from laboratory to and technician to technician, it is recommended that all operators achieve precision below these design goals before reporting results:

Pool	Intra Assay %CV	Inter Assay %CV
Low	~12%	~10%
High	~10%	~10%

Dilutional Linearity

The linearity of the kit was assayed by testing samples spiked with appropriate concentration of E.coli HCP and their serial dilutions. The results were demonstrated by percentage of calculated concentration to the expectation.

Sample	1:2	1:4	1:8
Cell Culture Supernatant (n=10)	91-105%	92-106%	90-111%

Safety Precautions:

- **This kit is For Research Use only.** Follow the working instructions carefully.
- The expiration dates stated on the kit are to be observed. The same relates to the stability stated for reagents

- Do not use or mix reagents from different lots.
- Do not use reagents from other manufacturers.
- Avoid time shift during pipetting of reagents.
- All reagents should be kept in the original shipping container.
- Some of the reagents contain small amount of sodium azide (< 0.1 % w/w) as preservative. They must not be swallowed or allowed to come into contact with skin or mucosa.
- Source materials maybe derived from body fluids or organs used in the preparation of this kit were tested and found negative for HBsAg and HIV as well as for HCV antibodies. However, no known test guarantees the absence of such viral agents. Therefore, handle all components and all patient samples as if potentially hazardous.
- Since the kit contains potentially hazardous materials, the following precautions should be observed
- Do not smoke, eat or drink while handling kit material
- Always use protective gloves
- Never pipette material by mouth
- Wipe up spills promptly, washing the affected surface thoroughly with a decontaminant.
- In any case GLP should be applied with all general and individual regulations to the use of this kit.



Typical Example of a Work List

Well #	Contents	Absorbance at 450nm	Mean Absorbance	Interpolated Concentration
1A	Standard No.1			
2A	Standard No.1			
1B	Standard No.2			
2B	Standard No.2			
1C	Standard No.3			
2C	Standard No.3			
1D	Standard No.4			
2D	Standard No.4			
1E	Standard No.5			
2E	Standard No.5			
1F	Standard No.6			
2F	Standard No.6			
1G	Standard No.7			
2G	Standard No.7			
1H	Sample			
2H				
3A	Sample			
4A				
3B	Sample			
4B				

LIMITED WARRANTY

Krishgen Biosystems does not warrant against damages or defects arising in shipping or handling, or out of accident or improper or abnormal use of the Products; against defects in products or components not manufactured by Krishgen Biosystems, or against damages resulting from such non-Krishgen Biosystems made products or components. Krishgen Biosystems passes on to customer the warranty it received (if any) from the maker thereof of such non Krishgen made products or components. This warranty also does not apply to Products to which changes or modifications have been made or attempted by persons other than pursuant to written authorization by Krishgen Biosystems.

THIS WARRANTY IS EXCLUSIVE. The sole and exclusive obligation of Krishgen Biosystems shall be to repair or replace the defective Products in the manner and for the period provided above. Krishgen Biosystems shall not have any other obligation with respect to the Products or any part thereof, whether based on contract, tort, and strict liability or otherwise. Under no circumstances, whether based on this Limited Warranty or otherwise, shall Krishgen Biosystems be liable for incidental, special, or consequential damages.

This Limited Warranty states the entire obligation of Krishgen Biosystems with respect to the Products. If any part of this Limited Warranty is determined to be void or illegal, the remainder shall remain in full force and effect.

Krishgen Biosystems. 2025

THANK YOU FOR USING A KRISHGEN PRODUCT!

KRISHGEN BIOSYSTEMS®, GENLISA®, DHARMAPLEX™, GENBULK™, GENLISA™, KRISHZYME®, KRISHGEN®, KRIBIOLISA®, KRISHPLEX®, TITANIUM®, QUALICHEK® are registered trademarks of KRISHGEN BIOSYSTEMS. ©KRISHGEN BIOSYSTEMS. ALL RIGHTS RESERVED.

KRISHGEN BIOSYSTEMS | OUR REAGENTS | YOUR RESEARCH |

SYMBOLS KEY

	Coated Microtiter Plate (12 x 8 wells)
	Standard
	Conjugate Horseradish Peroxidase
	Standard Diluent
	Assay Diluent
	(10X) Wash Buffer
	TMB Substrate
	Stop Solution
	Consult Instructions for Use
	Catalog Number
	Expiration Date
	Storage Temperature