

# KRIBIOLISA™ Human SSTR2B ELISA

**REF** : KBGT906

Ver 1.0

**RUO**

Enzyme Immunoassay for the Quantitative Detection of human SSTR2B in human serum, plasma and biological fluids.

|            |                              |            |                                       |
|------------|------------------------------|------------|---------------------------------------|
| <b>RUO</b> | <b>For Research Use Only</b> | <b>REF</b> | <b>Catalog Number</b>                 |
|            | <b>Store At</b>              | <b>LOT</b> | <b>Batch Code</b>                     |
|            | <b>Manufactured By</b>       |            | <b>Biological Risk</b>                |
|            | <b>Expiry Date</b>           |            | <b>Consult Operating Instructions</b> |

*For Laboratory Use Only. Purchase does not include or carry the right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of KRISHGEN BioSystems is strictly prohibited.*

**REF** KBGT906

96 tests

**KRISHGEN BioSystems**

For US/Europe Customers: toll free +1(888)-970-0827 | tel +1(562)-568-5005

For Asia/India Customers: +91(22)-49198700

Email: sales@krishgen.com | <http://www.krishgen.com>

**Introduction:**

Monoclonal and bispecific antibodies targeting GPRC5D, Claudins (Claudin 6 and Claudin 18), SSTR2, and CXCR4 have shown successful results in CAR-T cell therapy at the preclinical and clinical stages.

Somatostatin receptor type 2 is a protein that in humans is encoded by the SSTR2 gene. The SSTR2 gene is located on chromosome 17 on the long arm in position 25.1 in humans. The somatostatin receptor 2 (SSTR2), which belongs to the G-protein coupled receptor family, is a protein which is most highly expressed in the pancreas (both alpha- and beta-cells), but also in other tissues such as the cerebrum and kidney and in lower amount in the jejunum, colon and liver. In the pancreas, after binding to somatostatin, it inhibits the secretion of peptide hormones from pancreatic islets. During development, it stimulates neuronal migration and axon outgrowth.

The somatostatin receptor 2 is expressed in most tumors. Patients with neuroendocrine tumors that over-express the somatostatin receptor 2 have an improved prognosis. Somatostatin receptor 2 also has the ability to stimulate apoptosis in many cells including cancer cells. The somatostatin receptor 2 is also being looked at as a possible target in cancer treatment for its ability to inhibit tumor growth.

KRISHGEN'S KRIBIOLISA™ Human SSTR2B uses SSTR2B as VLP (virus like particle) as their standards / calibrators. Virus-like particles (VLPs) are nanoscale particles formed by self-assembly of viral capsid proteins, approximately 100-300 nm in diameter, which lack the viral genetic material, can't replicate autonomously, and are safer during production. This ensures a high degree of accuracy and reproducibility in results obtained using the KRISHGEN ELISAs.

**Intended Use:**

The KRIBIOLISA™ Human SSTR2B ELISA kit is specifically designed for the quantitative detection of SSTR2B in human serum, plasma, tissue homogenates, cell lysates and biological fluids.

**Principle:**

The method employs indirect capture antibody sandwich ELISA technique. Monoclonal Anti-SSTR2B is pre-coated onto the microwells. Samples and controls are pipetted into microwells and SSTR2B present in the sample are bound by the antibodies. Then Anti-Human IgG:HRP Conjugate is pipetted and incubated to form a complex. After washing to remove any non-specific binding, the substrate solution (TMB) is added to microwells and color develops proportionally to the amount of SSTR2B present in the sample. Color development is then stopped by addition of stop solution. Absorbance is measured at 450 nm. The presence or concentration of virus / antigen in samples is determined relative to supplied controls.

**Materials Provided:**

| Part                                | Description   | Qty          |
|-------------------------------------|---|--------------|
| Anti-SSTR2B Coated Microtiter Plate | 96 well polystyrene microplate (12 strips of 8 wells) coated with monoclonal antibody to SSTR2B.                      | 1 x 96 wells |
| SSTR2B Standard                     | SSTR2B VLPs in a buffered protein base and preservative sodium azide < 0.01% (concentrated, lyophilized)              | 1 vial       |
| Anti Human IgG:HRP Conjugate        | Anti Human IgG:HRP with protein stabilizer and preservatives 0.02% methylisothiazolone and 0.02% bromonitrodiroxane.  | 12 ml        |
| (1X) Sample Diluent                 | Buffered protein base with preservative sodium azide < 0.01%  | 2 x 50 ml    |
| (1X) Standard Diluent               | Buffered protein base with 1:2000 dilution human serum and preservative sodium azide < 0.01%                          | 10 ml        |
| (20X) Wash Buffer                   | 20-fold concentrated solution of buffered surfactant with preservative thiomersol < 0.01%. May turn yellow over time. | 25 ml        |
| TMB Substrate                       | Stabilized Chromogen  | 12 ml        |
| Stop Solution                       | 0.73M Phosphoric Acid   | 12 ml        |
| Instruction Manual                  |   | 1 no         |

**Materials to be provided by the End-User:**

1. Microplate Reader able to measure absorbance at 450 nm.
2. Adjustable pipettes to measure volumes ranging from 50 ul to 1000 ul.
3. Deionized (DI) water.
4. Wash bottle or automated microplate washer.
5. Tubes to prepare standard/sample dilutions.
6. Timer.
7. Absorbent paper.

**Storage Information:**

1. All components are to be stored at 2-8°C
2. Before using, bring all components to room temperature (18-25°C). Upon assay completion return all components to appropriate storage conditions.

**Health Hazard Warnings:**

1. Reagents that contain preservatives may be harmful if ingested, inhaled or absorbed through the skin. Refer to the MSDS online for details.
2. To reduce the likelihood of blood-borne transmission of infectious agents, handle all plasma in accordance with NCCLS regulations.

**Specimen Collection and Handling:**

Blood is taken by venipuncture. Serum is separated after clotting by centrifugation. Repeated freezing and thawing should be avoided. If samples are to be used for several assays, initially aliquot samples and keep at -20°C.

**Sample Preparation and Storage:**

Blood is taken by venipuncture. Serum is separated after clotting by centrifugation. Plasma can be used, too. Lipaemic, hemolytic or contaminated samples should not be run. Repeated freezing and thawing should be avoided. If samples are to be used for several assays, initially aliquot samples and keep at -20°C.

**Tissue Homogenates-** As hemolysis blood has relation to the assay results, it is necessary to remove residual blood by washing tissue with pre-coating PBS buffer (0.01M, pH=7.4). Mince tissue after weighing it and get it homogenized in PBS (the volume depends on the weight of the tissue. Normal 9 ml PBS would be appropriate to 1 gram tissue pieces. Some protease inhibitors are recommended to add into the PBS) with a glass homogenizer or ice. To further break the cells, you can sonicate the suspension with an ultrasonic cell disruptor or subject it to freeze-thaw cycles. The homogenates are then centrifuged for 5 minutes at 5000xg to get the supernatant. The total protein concentration was determined by BCA kit and the total protein concentration of each pore sample should not exceed 0.3 mg,

**Cell Culture Supernatant-** Centrifuge supernatant for 20 minutes at 1000xg at 2-8°C to remove insoluble impurity and cell debris. Collect the clear supernatant and carry out the assay immediately.

**Cell Culture Lysate-** Commercial RIPA kits are recommended to follow the instructions provided. Generally 0.5 ml RIPA lysis buffer would be appropriate to 2x10(6) cells, DNA must be removed. The total protein concentration was determined by BCA kit and the total protein concentration of each pore sample should not exceed 0.3 mg.

**Cell Culture Supernatant -** If necessary, centrifuge to remove debris prior to analysis. Samples can be stored at -20°C or -80°C. Avoid repeated freeze-thaw cycles.

**Preparation Before Use:**

Allow samples to reach room temperature prior to assay. Take care to agitate patient samples gently in order to ensure homogeneity.

**Serum and Plasma Test Sample Preparation** - Samples have to be diluted **1:1000 (v/v)**, e.g. for **1:1000 (1 ul sample + 999 ul Sample Diluent)** prior to assay. The samples may be kept at 2 - 8°C for up to three days. Long-term storage requires -20°C.

**Tissue Homogenate and Cell Culture Sample Preparation** - The user should estimate the concentration of target protein in the test sample, and select a proper dilution factor to make the diluted target protein concentration fall in the optimal detection range of the kit. Dilute the sample with the provided diluent, and several trials may be necessary. The test sample must be well mixed with the diluent. If samples are expected to have very high concentrations of the analyte, dilute the samples with PBS (pH 7.4) first and then further dilute with the Sample Diluent.

#### Reagent Preparation (all reagents should be diluted immediately prior to use):

1. Label any aliquots made with the kit Lot No and Expiration date and store it at appropriate conditions mentioned.
2. Bring all reagents to Room temperature before use.
3. To make (1X) Wash Buffer; dilute 25 ml of (20X) Wash Buffer in 475 ml of DI water.
4. **Standards Preparation:** Thaw the original concentrated Standard vial. Please check the table for the standard range calculations. Use the Standard Diluent as the Zero Standard (Standard No.0).

| Standard Concentration | Standard Vial     | Dilution Particulars  |
|------------------------|-------------------|---|
| 5000 ng/ml             | Original Standard | Original Standard provided in the Kit + 1 ml of Standard Diluent(1X)    |
| 2500 ng/ml             | Standard No.6     | 500 ul Reconstituted Standard (5000 ng/ml)+500 ul Standard Diluent (1X) |
| 1250 ng/ml             | Standard No.5     | 500 ul Standard No.6 + 500 ul Standard Diluent (1X)                     |
| 625 ng/ml              | Standard No.4     | 500ul Standard No.5+ 500 ul Standard Diluent (1X)                       |
| 312.5 ng/ml            | Standard No.3     | 500 ul Standard No.4 + 500 ul Standard Diluent (1X)                     |
| 156.25 ng/ml           | Standard No.2     | 500 ul Standard No.3 + 500 ul Standard Diluent (1X)                     |
| 78.125 ng/ml           | Standard No.1     | 500 ul Standard No.2 + 500 ul Standard Diluent (1X)                     |
| 0 ng/ml                | Standard No.0     | Only Standard Diluent (1X)  |

Use the Standards as soon as possible upon reconstitution. Discard balance standard after use.

#### Procedural Notes:

1. In order to achieve good assay reproducibility and sensitivity, proper washing of the plates to remove excess un-reacted reagents is essential.
2. If the SSTR2B concentration of the undiluted sample is less than the diluted sample, this may be indicative of the Hook Effect. To overcome Hook Effect samples to be assayed should be sufficiently diluted with our recommended diluent.
3. Avoid assay of Samples containing Sodium Azide (NaN<sub>3</sub>), as it could destroy the HRP activity resulting in under-estimation of the amount of the SSTR2B.
4. It is recommended that all the Standards and Samples be assayed in duplicates.
5. Maintain a repetitive timing sequence from well to well for all the steps to ensure that the incubation timings are same for each well.
6. The plates should be read within 30 minutes after adding the Stop Solution.
7. Make a work list in order to identify the location of Standards and Samples.



#### Assay Procedure:

1. It is strongly recommended that all Standards and Samples be run in duplicates. A standard curve is required for each assay. All steps must be performed at 37°C
2. Pipette **100 ul** of **prepared Standards or diluted Samples** into the respective wells
3. Cover the plate and incubate for 60 minutes at 37°C

4. Aspirate and wash plate 4 times with **Wash Buffer (1X)** and blot residual buffer by firmly tapping plate upside down on absorbent paper. Wipe off any liquid from the bottom outside of the microtiter wells as any residue can interfere in the reading step.
5. Pipette **100 ul** of **Anti-Human IgG:HRP Conjugate** into the respective wells.
6. Cover the plate and incubate for 60 minutes at 37°C.
7. Aspirate and wash plate 4 times with **Wash Buffer (1X)** same as in step 4.
8. Add **100 ul** of **TMB Substrate** in each well.
9. Incubate the plate at 37°C for 30 minutes in dark. DO NOT SHAKE or else it may result in higher backgrounds and worse precision. Positive wells should turn bluish in color.
10. Pipette out **100 ul** of **Stop Solution**. Wells should turn from blue to yellow in color.
11. Read the absorbance at 450 nm with a microplate reader.

#### **Calculation of Results:**

Determine the Mean Absorbance for each set of duplicate or triplicate Standards and Samples. Using Semi-Log graph paper, plot the average value (absorbance 450 nm) of each standard on the Y-axis versus the corresponding concentration of the standards on the X-axis. Draw the best fit curve through the standard points. To determine the unknown SSTR2B concentrations, find the unknown's Mean Absorbance value on the Y-axis and draw a horizontal line to the standard curve. At the point of intersection, draw a vertical line to the X-axis and read the SSTR2B Concentration. If samples were diluted, multiply by the appropriate dilution factor.

Software which is able to generate a cubic spline curve-fit or a 4-PL (2<sup>nd</sup> order) is best recommended for automated results.

#### **Note:**

It is recommended to repeat the assay at a different dilution factor in the following cases:

- If the sample absorbance value is below the first standard.
- If the absorbance value is equivalent or higher than the 2,500 ng/ml standard.

#### **Quality Control**

It is recommended that for each laboratory assay appropriate quality control samples in each run to be used to ensure that all reagents and procedures are correct.

#### **Performance Characteristics of the Kit:**

This kit has been validated as per EMA/FDA guidelines in line with ICH Code for Harmonization of Biological Assays.

#### **Sensitivity:**

**Limit Of Quantification:** It is defined as the lowest detectable concentration corresponding to a signal of Mean of '0' standard plus 2\* SD.

10 replicates of '0' standards were evaluated and the LOD was found to be ~50 ng/ml

#### **Specificity:**

The antibodies used in the kit are polyclonal antibodies specific for SSTR2B. The standards / calibrators used in the kit are VLPs to offer higher degree of accuracy and reproducibility.

**Precision:**

Precision is defined as the percent coefficient of variation (%CV) i.e. standard deviation divided by the mean and multiplied by 100. Assay precision was determined by both intra (n=5 assays) and inter assay (n=5 assays) reproducibility on two pools with low (78.125 ng/ml), medium (625 ng/ml) and high (2,500 ng/ml) concentrations. While actual precision may vary from laboratory to laboratory and technician to technician, it is recommended that all operators achieve precision below these design goals before reporting results.

| Pool   | Intra Assay %CV | Inter Assay %CV |
|--------|-----------------|-----------------|
| Low    | <10%            | <12%            |
| Medium | <5%             | <8%             |
| High   | <5%             | <8%             |

**Safety Precautions:**

- **This kit is for Research Use only.** Follow the working instructions carefully.
- The expiration dates stated on the kit are to be observed. The same relates to the stability stated for reagents
- Do not use or mix reagents from different lots.
- Do not use reagents from other manufacturers.
- Avoid time shift during pipetting of reagents.
- All reagents should be kept in the original shipping container.
- Some of the reagents contain small amount of sodium azide (< 0.1 % w/w) as preservative. They must not be swallowed or allowed to come into contact with skin or mucosa.
- Source materials maybe derived from human body fluids or organs used in the preparation of this kit were tested and found negative for HBsAg and HIV as well as for HCV antibodies. However, no known test guarantees the absence of such viral agents. Therefore, handle all components and all patient samples as if potentially hazardous.
- Since the kit contains potentially hazardous materials, the following precautions should be observed
- Do not smoke, eat or drink while handling kit material
- Always use protective gloves
- Never pipette material by mouth
- Wipe up spills promptly, washing the affected surface thoroughly with a decontaminant.
- In any case GLP should be applied with all general and individual regulations to the use of this kit.



## SCHEMATIC ASSAY PROCEDURE


1. Remove all components, 30 minutes before adding into the assay plate.



2. Avoid repeated cool-thaw of the components as there will be a loss of activity and this can affect the results.



3. Pipette 100 ul prepared Standards / diluted Samples into each well.

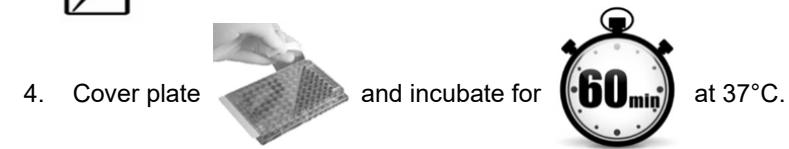

5. Aspirate and wash wells 4 times with Wash Buffer (1X).

6. Pipette 100 ul Detection HRP conjugate into each well.

7. Cover plate and incubate for 60 min at 37°C.

8. Aspirate and wash wells 4 times with Wash Buffer (1X).

9. Pipette 100 ul TMB Substrate into each well.

10. Cover plate and incubate for 30 min at 37°C.

11. Pipette 100 ul Stop Solution into each well.

12. Read absorbance at 450nm with a microplate reader within 30 min of stopping reaction.

**Typical Example of a Work List**

| Well # | Contents     | Absorbance at 450nm | Mean Absorbance | ng/ml Anti-Haemophilus influenzae B equivalent |
|--------|--------------|---------------------|-----------------|--|
| 1A     | zero std     |                     |                 |  |
| 2A     | zero std     |                     |                 |  |
| 1B     | 78.125 ng/ml |                     |                 |  |
| 2B     | 78.125 ng/ml |                     |                 |  |
| 1C     | 156.25 ng/ml |                     |                 |  |
| 2C     | 156.25 ng/ml |                     |                 |  |
| 1D     | 312.50 ng/ml |                     |                 |  |
| 2D     | 312.50 ng/ml |                     |                 |  |
| 1E     | 625 ng/ml    |                     |                 |  |
| 2E     | 625 ng/ml    |                     |                 |  |
| 1F     | 1250 ng/ml   |                     |                 |  |
| 2F     | 1250 ng/ml   |                     |                 |  |
| 1G     | 2500 ng/ml   |                     |                 |  |
| 2G     | 2500 ng/ml   |                     |                 |  |
| 1H     | sample       |                     |                 |  |
| 2H     | sample       |                     |                 |  |
| 1I     | sample       |                     |                 |  |
| 2I     | sample       |                     |                 |  |

**LIMITED WARRANTY**

Krishgen Biosystems does not warrant against damages or defects arising in shipping or handling, or out of accident or improper or abnormal use of the Products; against defects in products or components not manufactured by Krishgen Biosystems, or against damages resulting from such non-Krishgen Biosystems made products or components. Krishgen Biosystems passes on to customer the warranty it received (if any) from the maker thereof of such non Krishgen made products or components. This warranty also does not apply to Products to which changes or modifications have been made or attempted by persons other than pursuant to written authorization by Krishgen Biosystems.

THIS WARRANTY IS EXCLUSIVE. The sole and exclusive obligation of Krishgen Biosystems shall be to repair or replace the defective Products in the manner and for the period provided above. Krishgen Biosystems shall not have any other obligation with respect to the Products or any part thereof, whether based on contract, tort, and strict liability or otherwise. Under no circumstances, whether based on this Limited Warranty or otherwise, shall Krishgen Biosystems be liable for incidental, special, or consequential damages.

This Limited Warranty states the entire obligation of Krishgen Biosystems with respect to the Products. If any part of this Limited Warranty is determined to be void or illegal, the remainder shall remain in full force and effect.

Krishgen Biosystems. 2023

**THANK YOU FOR USING KRISHGEN PRODUCT!**

KRISHGEN BIOSYSTEMS®, GENLISA®, DHARMAPLEX™, GENBULK™, GENLISA™, KRISHZYME®, KRISHGEN®, KRIBIOLISA®, KRISHPLEX®, TITANIUM®, QUALICHEK® are registered trademarks of KRISHGEN BIOSYSTEMS. ©KRISHGEN BIOSYSTEMS. ALL RIGHTS RESERVED.

KRISHGEN BIOSYSTEMS | OUR REAGENTS | YOUR RESEARCH |

## SYMBOLS KEY

|  |  |
|--|--|
|  | Anti-SSTR2B Coated Microtiter Plate (12x8 wells) |
|  | SSTR2B Standard                                  |
|  | Conjugate Horseradish Peroxidase                 |
|  | (1X) Sample Diluent                              |
|  | (1X) Standard Diluent                            |
|  | (20X) Wash Buffer                                |
|  | TMB Substrate                                    |
|  | Stop Solution                                    |
|  | Consult Instructions for Use                     |
|  | Catalog Number                                   |
|  | Expiration Date                                  |
|  | Storage Temperature                              |